
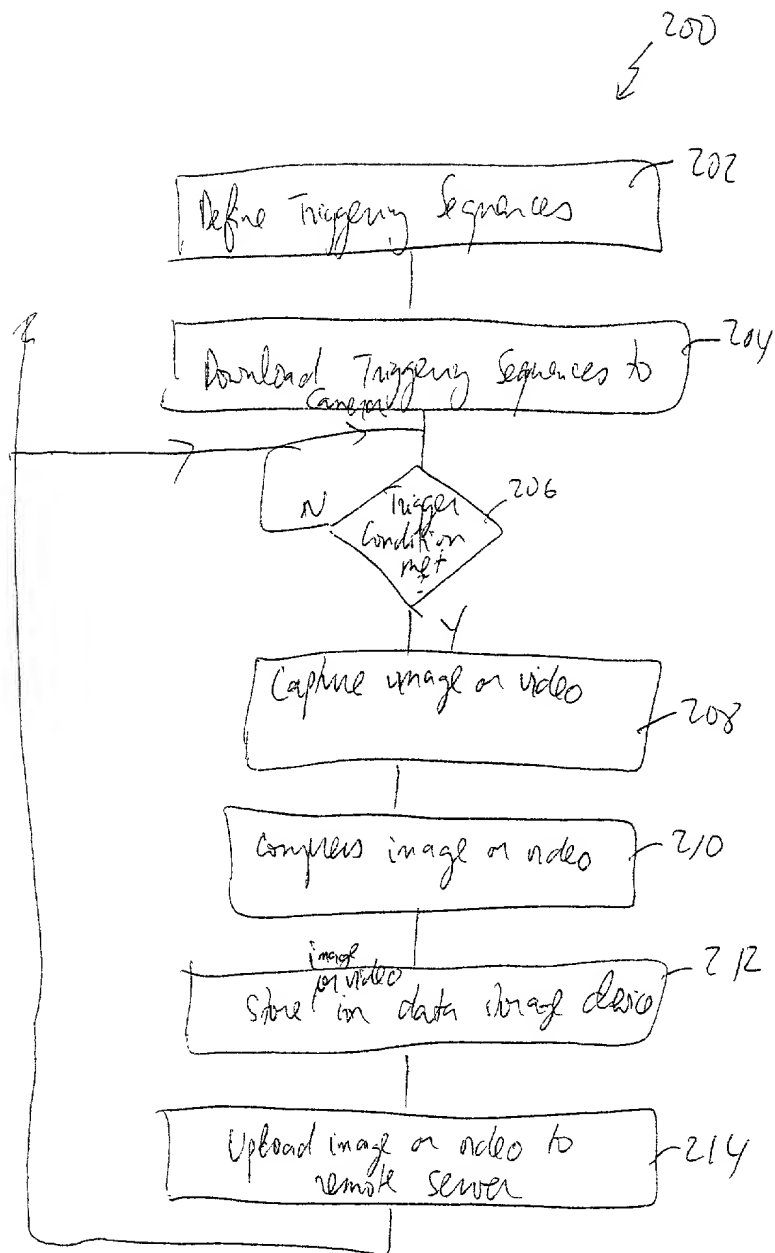


FIG 1

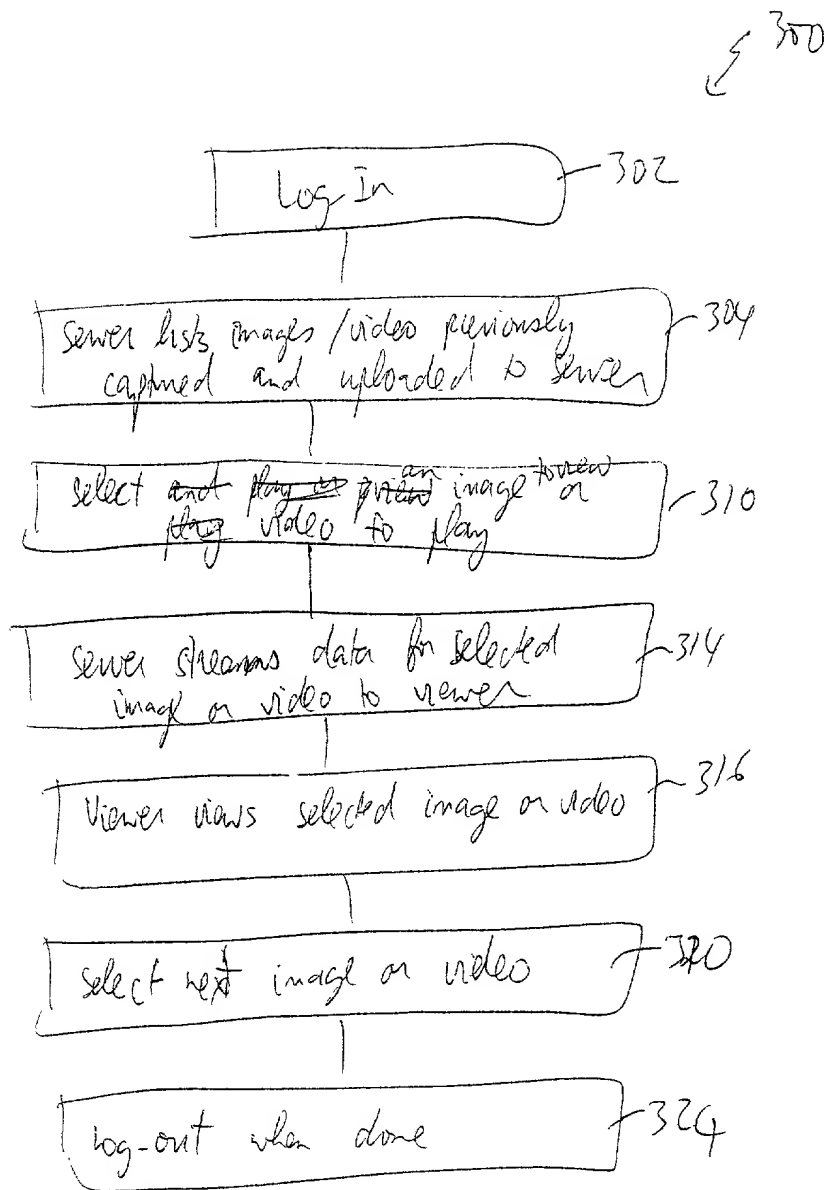

F. 2



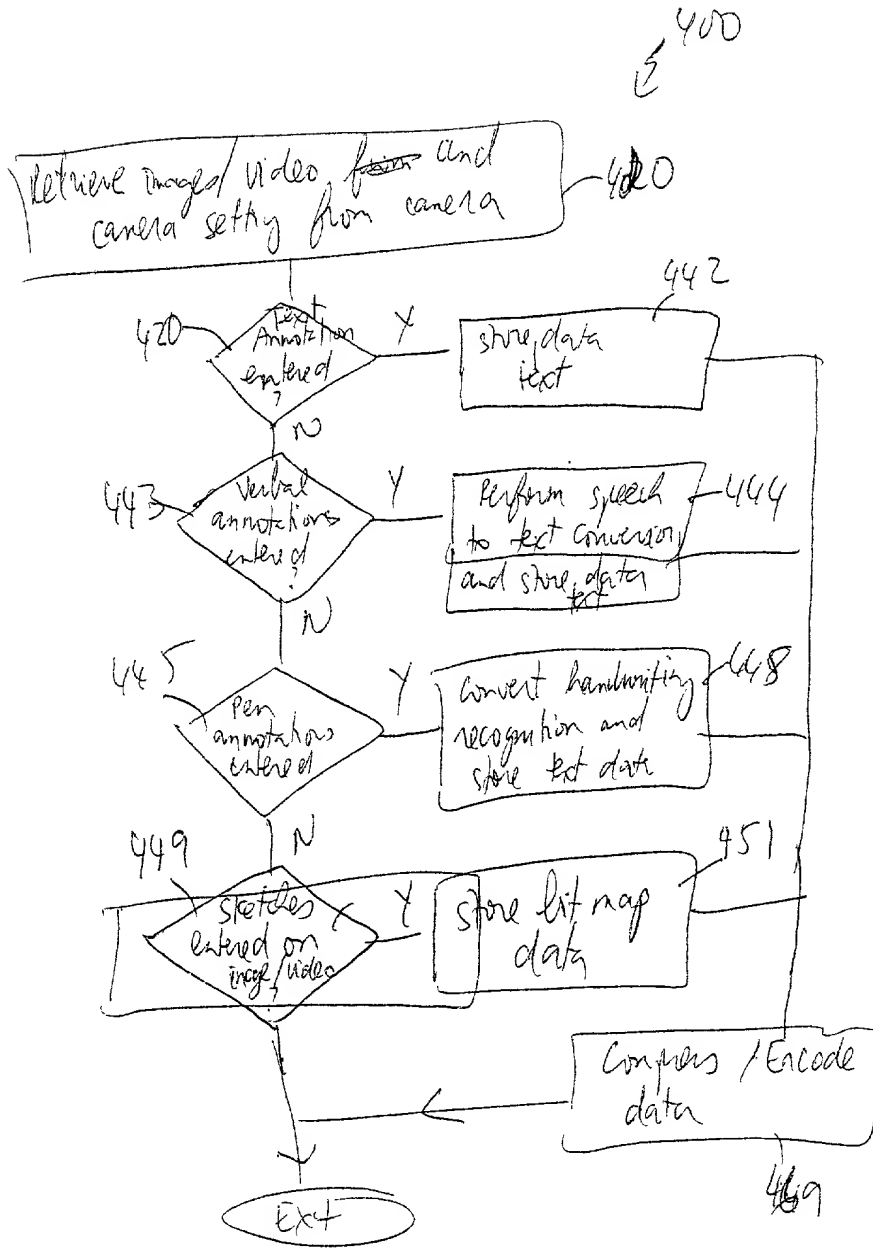


Fig. 4

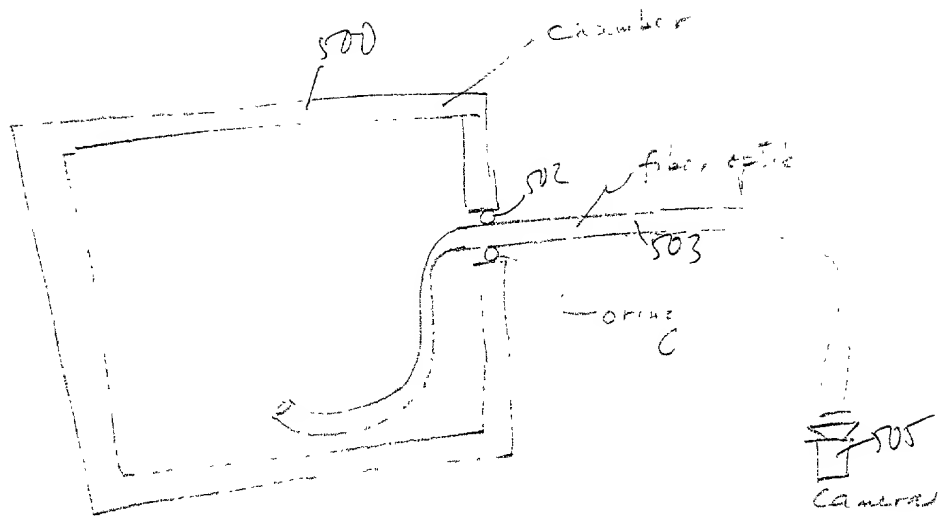
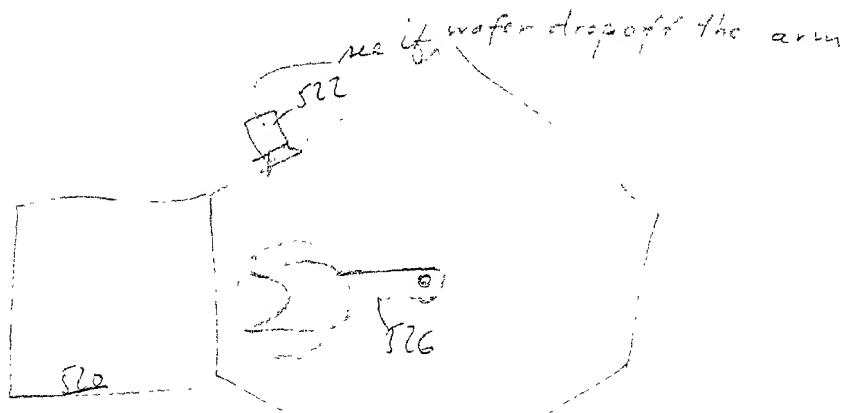
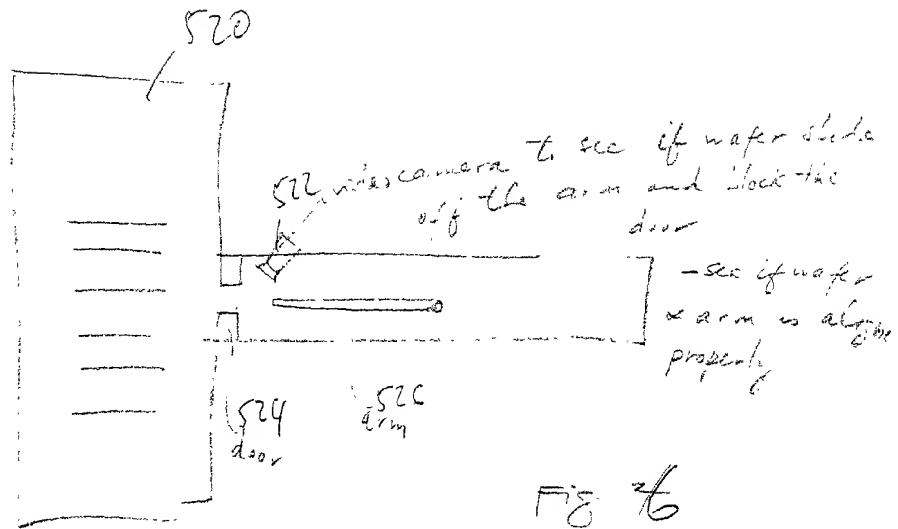


Fig 5.
Vacuum adapter for viewing inside the
chamber



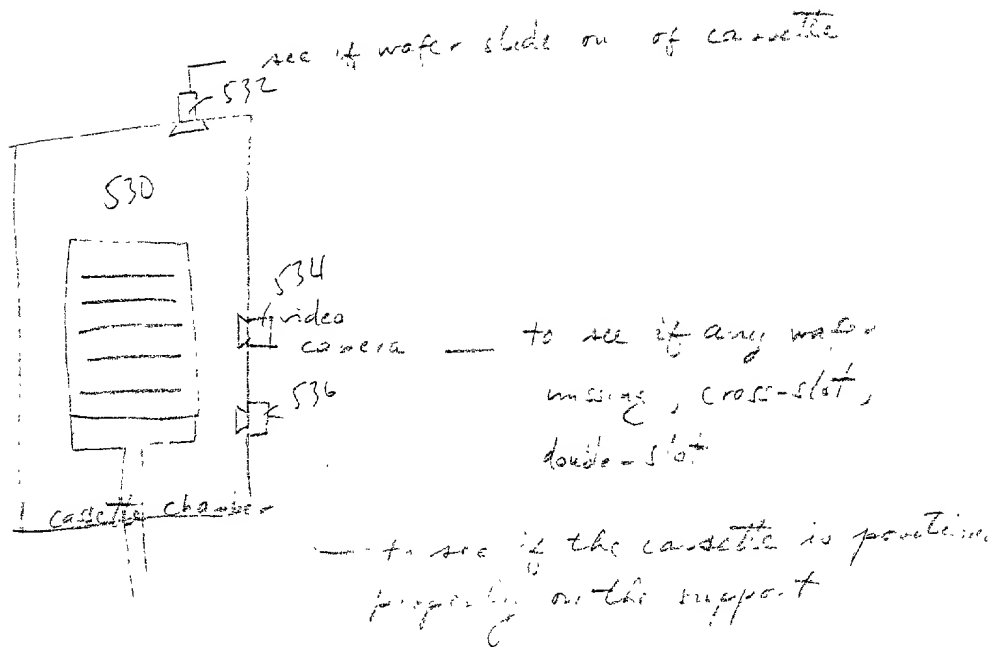


Fig 8

09765821.042301

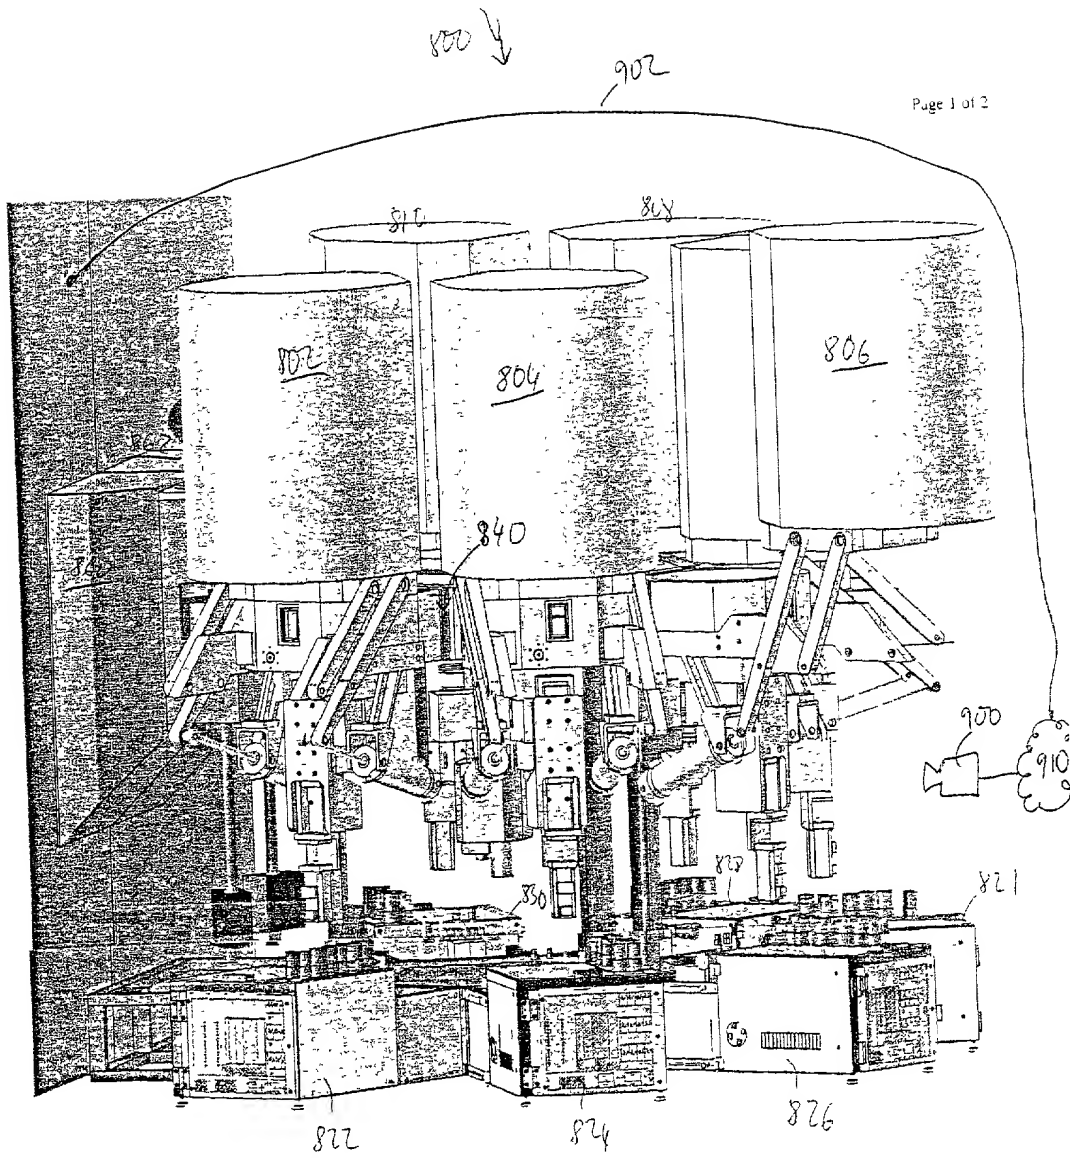


FIG 9